



**University of
Zurich** UZH

**Zurich Open Repository and
Archive**

University of Zurich
University Library
Strickhofstrasse 39
CH-8057 Zurich
www.zora.uzh.ch

Year: 2014

Patient specific implants (PSI) in reconstruction of orbital floor and wall fractures

Gander, Thomas ; Essig, Harald ; Metzler, Philipp ; Lindhorst, Daniel ; Dubois, Leander ; Rücker, Martin ;
Schumann, Paul

DOI: <https://doi.org/10.1016/j.jcms.2014.10.024>

Posted at the Zurich Open Repository and Archive, University of Zurich

ZORA URL: <https://doi.org/10.5167/uzh-102791>

Journal Article

Accepted Version

Originally published at:

Gander, Thomas; Essig, Harald; Metzler, Philipp; Lindhorst, Daniel; Dubois, Leander; Rücker, Martin; Schumann, Paul (2014). Patient specific implants (PSI) in reconstruction of orbital floor and wall fractures. *Journal of Cranio-Maxillofacial Surgery*, 43(1):126-130.

DOI: <https://doi.org/10.1016/j.jcms.2014.10.024>

Manuscript Number: JCMS-D-14-00437R2

Title: Patient specific Implants (PSI) in Reconstruction of Orbital Floor and Wall Fractures

Article Type: Original Paper

Keywords: Orbital Fractures; Patient specific Implants (PSI); Reconstruction, Computer-assisted surgery

Corresponding Author: Dr.Med. Thomas Gander, MD, DMD

Corresponding Author's Institution: Clinic for cranio-maxillofacial surgery, university hospital zürich

First Author: Thomas Gander, MD, DMD

Order of Authors: Thomas Gander, MD, DMD; Harald Essig, MD, DMD; Philipp Metzler, MD, DMD; Daniel Lindhorst, MD, DMD; Leander Dubois, MD, DMD; Martin Rücker, MD, DMD; Paul Schumann, MD, DMD

Abstract: Fractures of the orbital wall and floor can be challenging due to the demanding three-dimensional anatomy and limited intraoperative overview. Misfitting implants and inaccurate surgical technique may lead to visual disturbance and unaesthetic results. A new approach using individually manufactured titanium implants (KLS Martin, Group, Germany) for daily routine is presented in the current paper. Preoperative CT-scan data were processed in iPlan 3.0.5 (Brainlab, Feldkirchen, Germany) to generate a 3D-reconstruction of the affected orbit using the mirrored non-affected orbit as template and the extent of the patient specific implant (PSI) was outlined and three landmarks were positioned on the planned implant in order to allow easy control of the implant's position by intraoperative navigation. Superimposition allows the comparison of the postoperative result with the preoperative planning. Neither reoperation was indicated due to malposition of the implant and the ocular bulb nor visual impairments could be assessed. PSI allows precise reconstruction of orbital fractures by using a complete digital workflow and should be considered superior to manually bent titanium mesh implants.

Patient specific Implants (PSI) in Reconstruction of Orbital Floor and Wall Fractures

Thomas Gander MD, DMD¹

Harald Essig MD, DMD¹

Philipp Metzler MD, DMD¹

Daniel Lindhorst MD, DMD¹

Leander Dubois MD, DMD²

Martin Rücker MD, DMD¹

Paul Schumann MD, DMD¹

¹Department of Oral and Maxillofacial Surgery, University Hospital of Zürich, Zürich, Switzerland

²Department of Oral and Maxillofacial Surgery, University of Amsterdam, Amsterdam, Netherlands

Address of correspondence

Dr. med. Dr. med. dent. Thomas Gander
Department of Oral and Maxillofacial Surgery
University Hospital of Zürich
Frauenklinikstrasse 24
CH-8091 Zürich
Switzerland
Phone 0041442555062
Fax 0041442554179
Email: Thomas.Gander@usz.ch

No sources of support.

Dear Reviewers,

Thank you very much for your constructive comments and for suggesting our paper for publication. According to your comments we made the following changes in our manuscript:

Reviewer #1: Thank you very much for your pleasant comment.

Reviewer #2: Thank you very much for your constructive comments. PSI can easily be manually bent, of course in a limited extent, compared with standardized titanium meshes. The goal of treatment planning should be the perfect fit of the implant. As mentioned, only two implants had to be corrected in their extent by pincers. An adjustment by bending was not necessary, although, as mentioned above, this could be performed but should be avoided by meticulous planning. Long-term results will follow and more patients will be included in future studies. The figures 5 and 7 have been removed.

All changes were highlighted in the text by using red color. We hope that our manuscript is now suitable for publication and hope for acceptance.

Yours sincerely

Dr. Dr. Thomas Gander

Introduction

The orbital wall and floor are common sites of facial bone fracture and may cause serious functional impairment (Shin et al., 2013). Numerous cases of reconstructive implant use have been described in the literature (Strong et al., 2013; Gerressen et al., 2012). The repair of orbital wall and floor fractures is difficult due to the complexity of the anatomical region involved, and the limited intraoperative view. Meticulous imaging, and clinical examination, is indispensable for treatment planning, in order to restore orbital volume and shape. Ill-fitting implants and inaccurate surgical techniques may lead to visual disturbances and unaesthetic results (Ewers et al., 2005). Computer assisted three-dimensional (3D) treatment planning, and ready-to-use, individual titanium mesh implants, are routinely applied to achieve stable reconstruction and adequate postoperative results (Essig et al., 2013; Schramm et al., 2009). Contemporary standardized titanium meshes are manually adjusted to fit individual patients' polyamide models (Kozakiewicz and Szymor, 2013). We present a new approach employing customized, ready to use, patient-specific titanium implants (KLS Martin, Group, Germany), suitable for daily use. These easily manufactured and implemented, ready-made patient specific implants (PSI) allow for a more cost- and time-effective operating procedure.

Material and methods

Patients who underwent operations for orbital wall and/or floor fractures, between February 2014 and June 2014, were recruited, irrespective of their gender, age, trauma type or the presence of concomitant injuries. Informed consent was provided by all patients. Preoperative CT-scan data, with a slice thickness of 0.3 mm, were processed using the iPlan software package (ver. 3.0.5, Brainlab, Feldkirchen, Germany) to generate a 3D reconstruction of the affected orbit, using the mirrored non-affected orbit as a template. Correction of minor asymmetry was effected via the 3D smart shaper function. Accurate use of the 3D smart shaper is a key step in the planning process, and must be performed with caution to avoid discrepancies during subsequent implant placement (Figures 1-2). The parameters of the patient-specific implant are outlined, and three landmarks are positioned on the planned implants to allow for rapid and effective 3D control of the implant's position (Figures 3-5). Each planning step can be easily performed by any surgeon: no specialist, *a priori* knowledge of the software is beneficial.

Precise transfer of the 3D coordinates of the implant, from iPlan 3.0.5 to the manufacturing software (KLS Martin), represents an essential precondition of intraoperative control. STL data are then exported and approved for the purposes of implant manufacture. This procedure obviates the need for time-consuming integration of the dataset within the manufacturing software. Circumferential implant cushions should be created, although laser-sintered, individually manufactured implants (with a thickness of 0.3 mm) exhibit greater stiffness compared with manually adjusted titanium meshes and therefore allow for minor dimensioning of the implant (Ibrahim et al., 2009). Overextended implants can easily be reduced in extent by pincers **and manual adjustment is still possible, although to a lesser degree compared with standardized implants. The need of manual adjustment should be avoided by meticulous preoperative implant planning.**

Individually manufactured titanium implants are positioned using a retroseptal, transconjunctival approach (Figure 6). Application of a polydioxanon foil, which may

improve the surgeon's view by preventing fatty tissues from encroaching on to the operative site, was utilized in certain cases. The polydioxanon foil is removed following placement of the implant and prior to wound closure. Dental arch splints in dentulous patients, and mini screws placed in the calvarian bones of edentulous patients, were used as registration markers. Postoperative CT-scans were performed to assess implant position. Quality management was effected by importation and superimposition of the postoperative dataset (Figure 7). All patients underwent a pre- and post-operative ophthalmological examination.

Results

A total 12 patients were included. All patients underwent reconstruction of the orbital wall or orbital floor, via PSIs using intraoperative navigation, and in accordance with a transconjunctival, post-septal approach. In eight patients indication for surgery was imposed due to diplopia. Four patients underwent orbital reconstruction owing to profound defects or enophthalmos. The male to female ratio of the sample was 11:1, with a mean age of 53 years (range: 29-78 years). Major causes of orbital floor or wall fractures included industrial accidents and falls (Table 1).

In seven patients, dental splints were applied for intraoperative navigation purposes, in addition to dental cusps. In four patients navigation screws were employed in the calvaria, for intraoperative registration and navigation. CT scans were performed preoperatively, and the registration tools were introduced.

The time taken for digital planning ranged between 30-36 min: the manufacturing process took 4-6 days. All individually manufactured implants were placed without difficulty. Postoperative CT scans revealed accurate fitting of the PSI. No visual impairments were reported aside from double vision in terminal positions, which resolved during postoperative care. Reoperation was not required to reposition implants, or to correct displacement of the ocular bulb. In two cases intraoperative reduction of the implant, using pincers, was necessary due to overextension during computer-aided treatment planning. **Manual adjustment by bending was not necessary in any case.** Patients did not report sensations indicative of foreign bodies nor any visual impairment (Table 2).

Discussion

Orbital floor and wall fractures represent common skeletal, facial injuries (Rosado and de Vicente, 2012; Dimitroulis and Eyre, 1991): diplopia, enophthalmos and infra-orbital and optical nerve injuries are potential complications of orbital floor and wall fracture surgery (Brucoli et al., 2011). Safe, rapid, reproducible and precise procedures are required to avoid such issues. Computer-assisted surgery represents a key step towards safer practice, and has become a standard technique during the past few years, allowing for virtual surgery planning, simulation and intraoperative control (Essig et al., 2013; Schramm et al, 2009). New surgical methods, and improved implant designs and materials, have been introduced incrementally, in some cases with great success (Gierloff et al., 2012; Avashia et al., 2012; Ciprandi et al., 2012; Schumann et al., 2013). PSIs allow for the precise reconstruction of orbital fractures by means of a complete digital workflow. Manually bent titanium mesh implants will become less important. A precondition of the digital workflow is the transfer of the planning software's coordinates system into the manufacturing software, to avoid time-consuming and erroneous positioning of the virtual implant.

Correct positioning of the PSI can be verified using intraoperative navigation, to support the three virtually planned indentations incorporated in the manufactured implant (Schramm et al., 2009). The three planned indentations and their stored coordinates also serve as measuring points during the virtual planning process, thereby improving overall accuracy. The implant is digitally planned by the surgeon, with a focus on its extent and the position of the three landmarks. The coordinate system of the digital plan must be conserved during the entirety of the manufacturing process, to allow for accurate superimposition of the pre- and postoperative implant positions. Although PSIs are dimensionally more stable compared with manually bent titanium implants, a circumferential cushion is nonetheless recommended. Furthermore, stiffness in PSIs prevents implant deformation during placement, but still allows for minor, intraoperative corrections by pincers. Due to the increased stiffness of laser-sintered PSIs compared with conventional titanium meshes, precise preoperative planning is required to avoid interference during insertion of the PSI. Routinely incorporating postoperative results into preoperative virtual planning activities, and assessing implant positioning via superimposition, both represent ground-breaking advances in medical quality control.

Conclusion

PSIs simplify the reconstruction of orbital floor and wall fractures, and should be considered a more accurate alternative to manually bent titanium mesh implants. Automation allows for the application of safe, time-effective, daily procedures; accordingly, its use should be encouraged. Implant planning can be easily undertaken by any surgeon, and does not require specialized, software-specific knowledge.

As previously stated by the World Health Organization, PSIs should play a key role in daily routines, and furthermore should replace conventional implants by 2020. PSI for the reconstruction of orbital floor and wall fractures is now readily available.

More patients will be included in this study and long-term results will be gathered in the future to allow more funded statements.

Conflict of Interest Statement

All authors disclose any financial and personal relationships with other people or organisations that could inappropriately influence (bias) this work.

Funding

None.

References

Shin JW, Lim JS, Yoo G, Byeon JH: An analysis of pure blowout fractures and associated ocular symptoms. *J Craniofac Surg* 24:703-707, 2013.

Strong EB, Fuller SC, Wiley DF, Zumbansen J, Wilson MD, Metzger MC: Preformed vs intraoperative bending of titanium mesh for orbital reconstruction. *Otolaryngol Head Neck Surg* 149:60-66, 2013.

Gerressen M, Gillessen S, Riediger D, Hölzle F, Modabber A, Ghassemi A: Radiologic and facial morphologic long-term results in treatment of orbital floor fracture with flexible absorbable alloplastic material. *J Oral Maxillofac Surg* 70:2375-2385, 2012.

Ewers R, Schicho K, Undt G, Wanschitz F, Truppe M, Seemann R, Wagner A: Basic research and 12 years of clinical experience in computer-assisted navigation technology: a review. *Int J Oral Maxillofac Surg* 34:1-8, 2005.

Essig H, Dressel L, Rana M, Kokemueller H, Ruecker M, Gellrich NC: Precision of posttraumatic primary orbital reconstruction using individually bent titanium mesh with and without navigation: a retrospective study. *Head Face Med* 9: 18, 2013.

Schramm A, Suarez-Cunqueiro MM, Rücker M, Kokemueller H, Bormann KH, Metzger MC, Gellrich NC: Computer-assisted therapy in orbital and mid-facial reconstructions. *Int J Med Robot* 5:111-124, 2009.

Kozakiewicz M, Szymor P: Comparison of pre-bent titanium mesh versus polyethylene implants in patient specific orbital reconstructions. *Head Face Med* 29:32, 2013.

Ibrahim D, Broilo TL, Heitz C, de Oliveira MG, de Oliveira HW, Nobre SM, Dos Santos Filho JH, Silva DN: Dimensional error of selective laser sintering, three-dimensional printing and PolyJet models in the reproduction of mandibular anatomy. *J Craniomaxillofac Surg* 37:167-173, 2009.

Rosado P, de Vicente JC: Retrospective analysis of 314 orbital fractures. *Oral Surg Oral Med Oral Pathol Oral Radiol* 113:168-171, 2012.

Dimitroulis G, Eyre J: A 7-year review of maxillofacial trauma in a central London hospital. *Br Dent J* 20:300-302, 1991.

Brucoli M, Arcuri F, Cavenaghi R, Benech A: Analysis of complications after surgical repair of orbital fractures. *J Craniofac Surg* 22:1387-1390, 2011.

Gierloff M, Seeck NG, Springer I, Becker S, Kandzia C, Wiltfang J: Orbital floor reconstruction with resorbable polydioxanone implants. *J Craniofac Surg* 23:161-164, 2012.

Avashia YJ, Sastry A, Fan KL, Mir HS, Thaller SR: Materials used for reconstruction after orbital floor fracture. *J Craniofac Surg* 23: 1991-1997, 2012.

Ciprandi MT, Primo BT, Gassen HT, Closs LQ, Hernandez PA, Silva AN Jr: Calcium phosphate cement in orbital reconstructions. *J Craniofac Surg* 23: 145-148, 2012.

Schumann P, Lindhorst D, Wagner ME, Schramm A, Gellrich NC, Rücker M: Perspectives on resorbable osteosynthesis materials in craniomaxillofacial surgery. *Pathobiology* 80: 211-217, 2013.

Tables/Figures

Table 1 Patient data
Table 2 Results

Figure 1	Placement of the smart shaper in the required area
Figure 2	Adaption of the selected area with the smart shaper
Figure 3	Determination of the prospective implant's extent
Figure 4	Implant design
Figure 5	Intraoperative navigation for implant position control
Figure 6	Transconjunctival, post-septal PSI placement
Figure 7	Superimposition of the preoperative planning position upon the postoperative PSI position

The English in this document has been checked by at least two professional editors, both native speakers of English.

Table 1

Patient data	
Age in years, mean (Range)	53.08 (29-78)
Number of patients and gender	
Overall	12
Female	1
Male	11
Fracture types	
Orbital fracture simple *	5
Orbital fracture complex*	4
Combined Midface fracture	3
Course of accident	
Industrial accidents	3
Tumbles	4
Sport accidents	2
Syncope	1
Road accidents	1
Violence	1

* Simple = single wall fracture, complex = more than one wall

Table 2

Results	
Indication for surgery	
Double vision	8
Endophthalmos	3
Extent of defect without symptoms	1
Surgical access	
Transconjunctival, retroseptal	11
Transconjunctival, retrocaruncular	1
Navigation tool	
Dental splint	7
Dental cusps	1
Calvarian screws	4
Complications intra-/postoperative	
Misfitting implant	0
Overextent of implant	2
Underextent of implant	0
Orbital nerve injury	0
Foreign body sensation	0
Postoperative double vision temporarily	5
Postoperative double vision permanent	0
Variance implant position vs digital plan (mm)	
Minimal 0.3mm	
Maximum 1.6mm	

Figure 1
[Click here to download high resolution image](#)

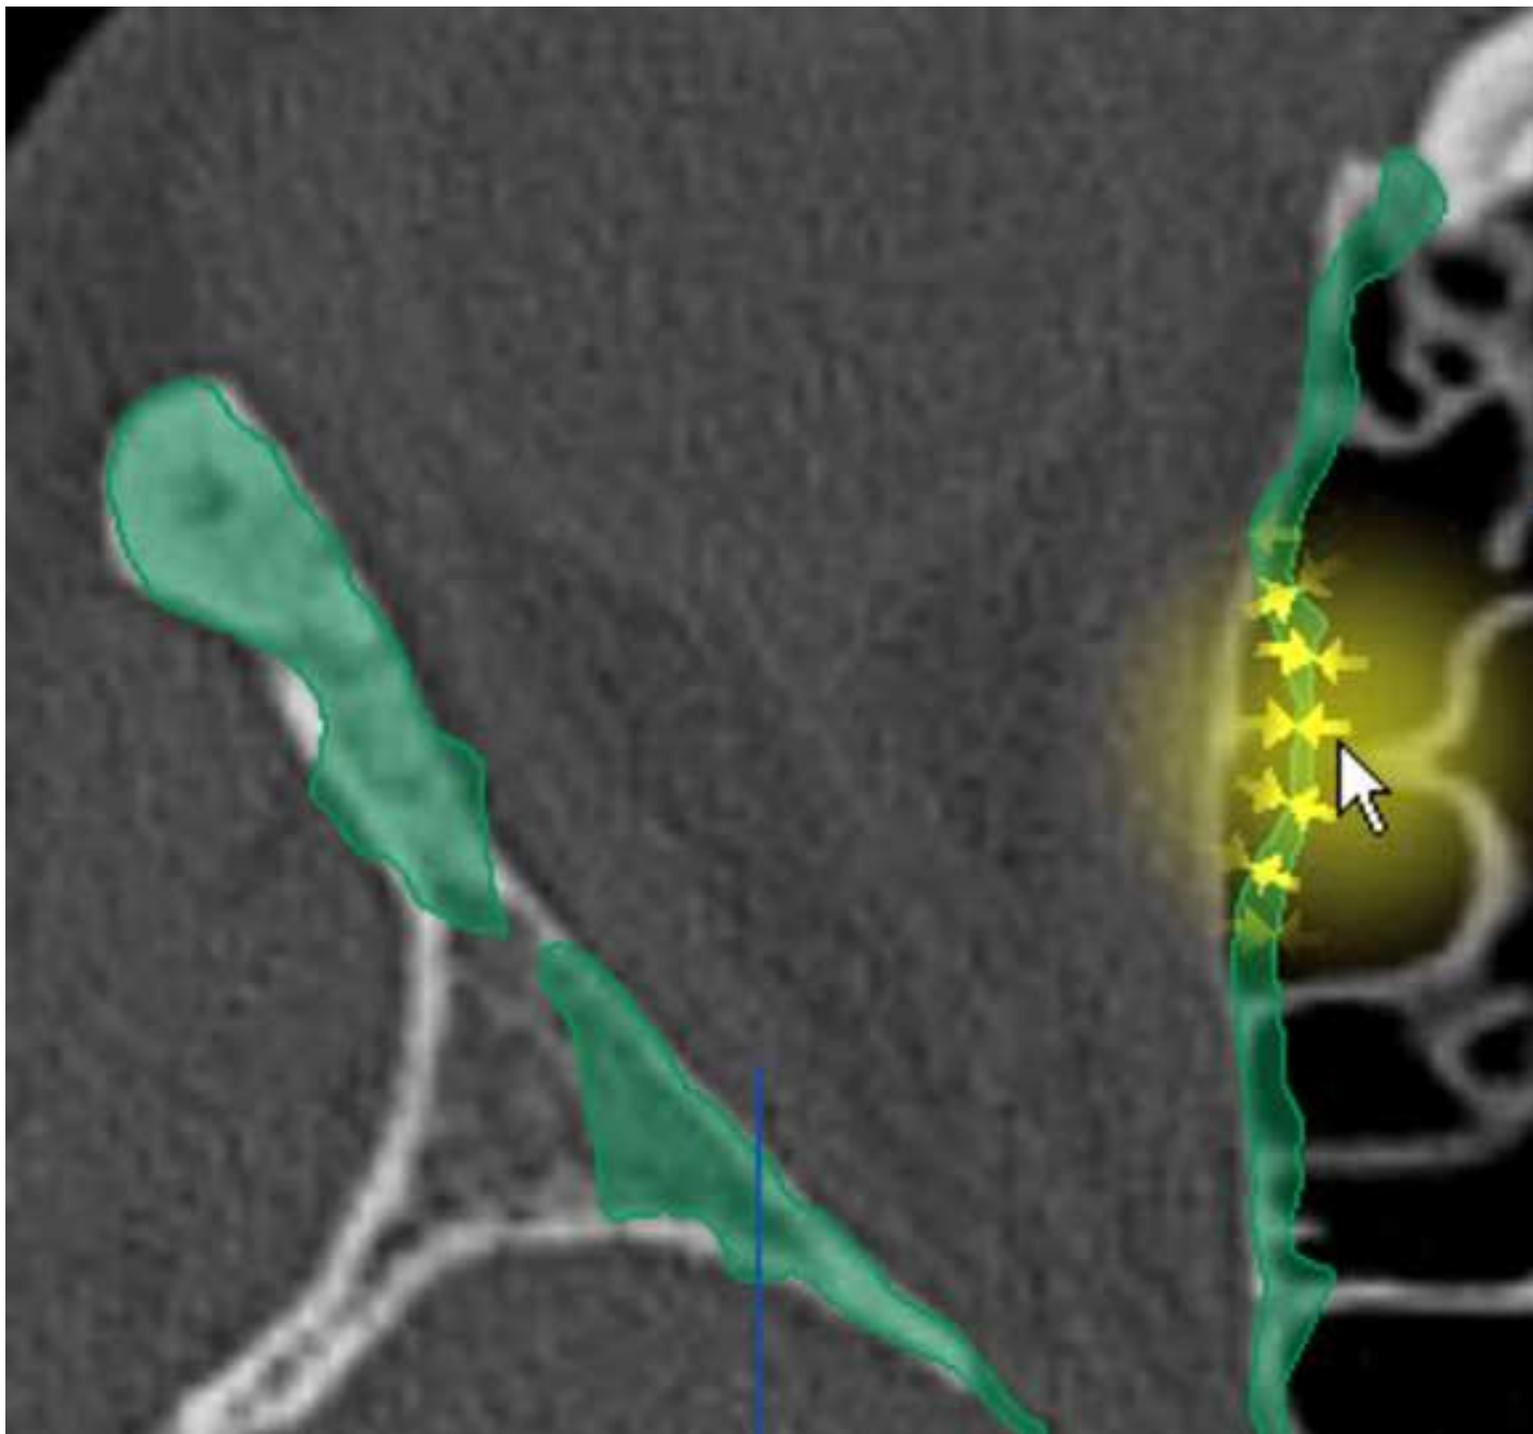


Figure 2
[Click here to download high resolution image](#)

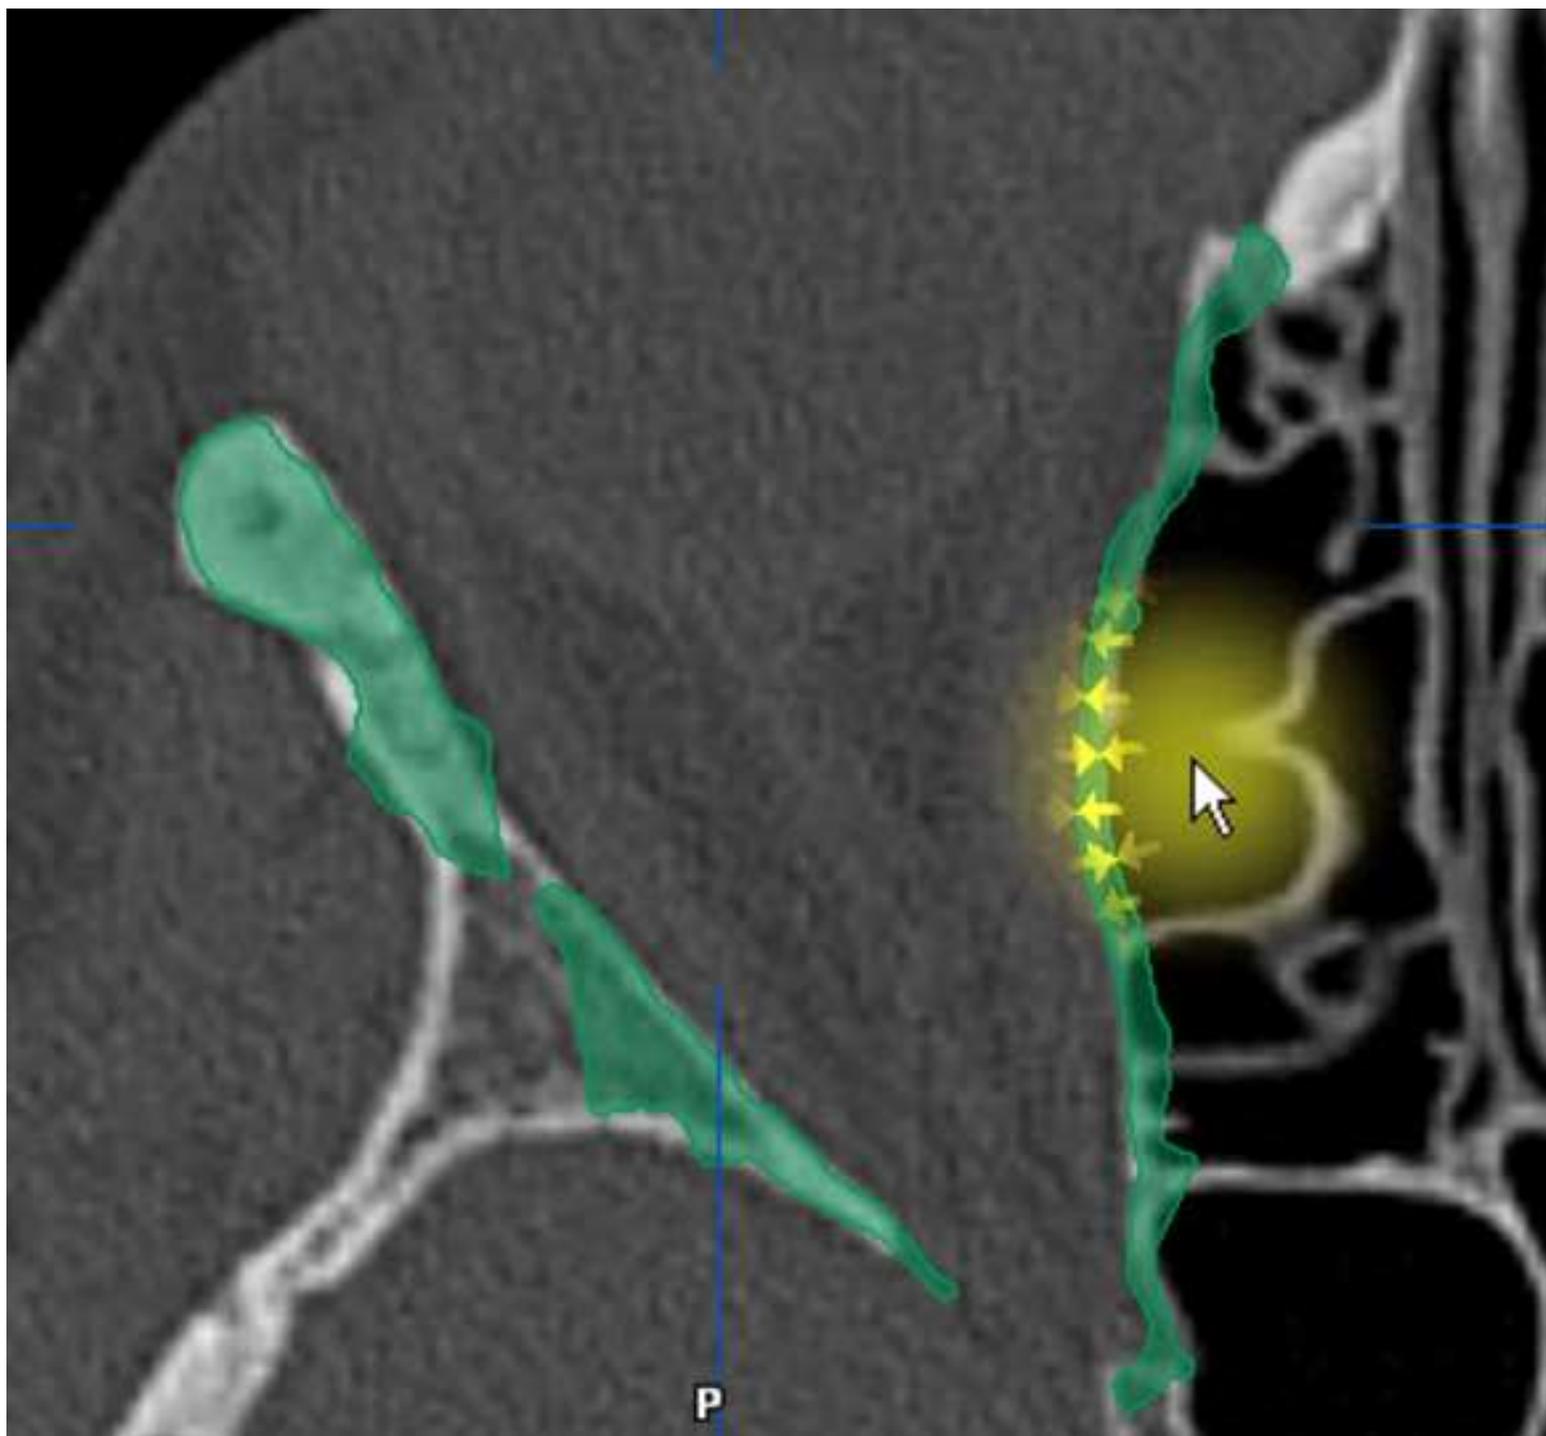


Figure 3
[Click here to download high resolution image](#)

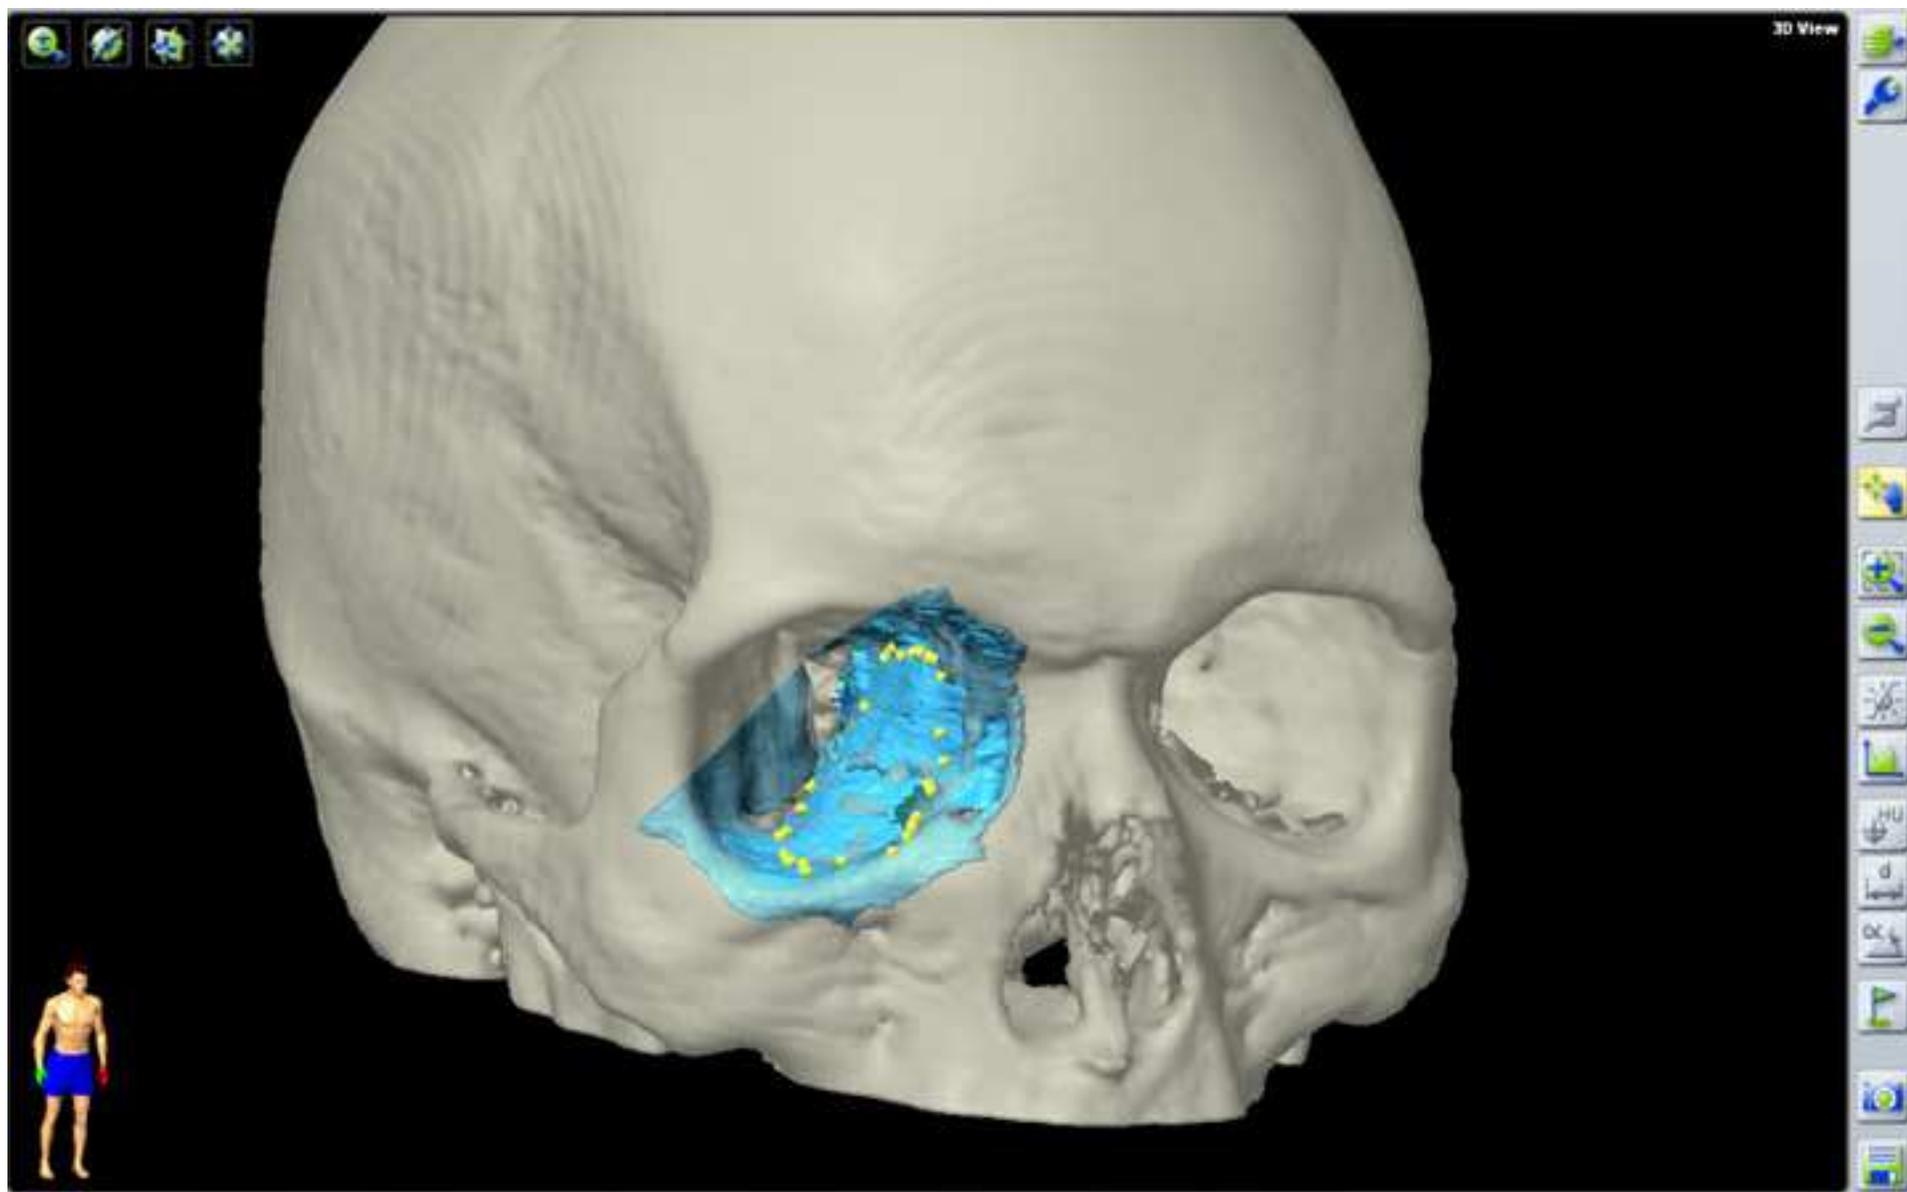


Figure 4
[Click here to download high resolution image](#)

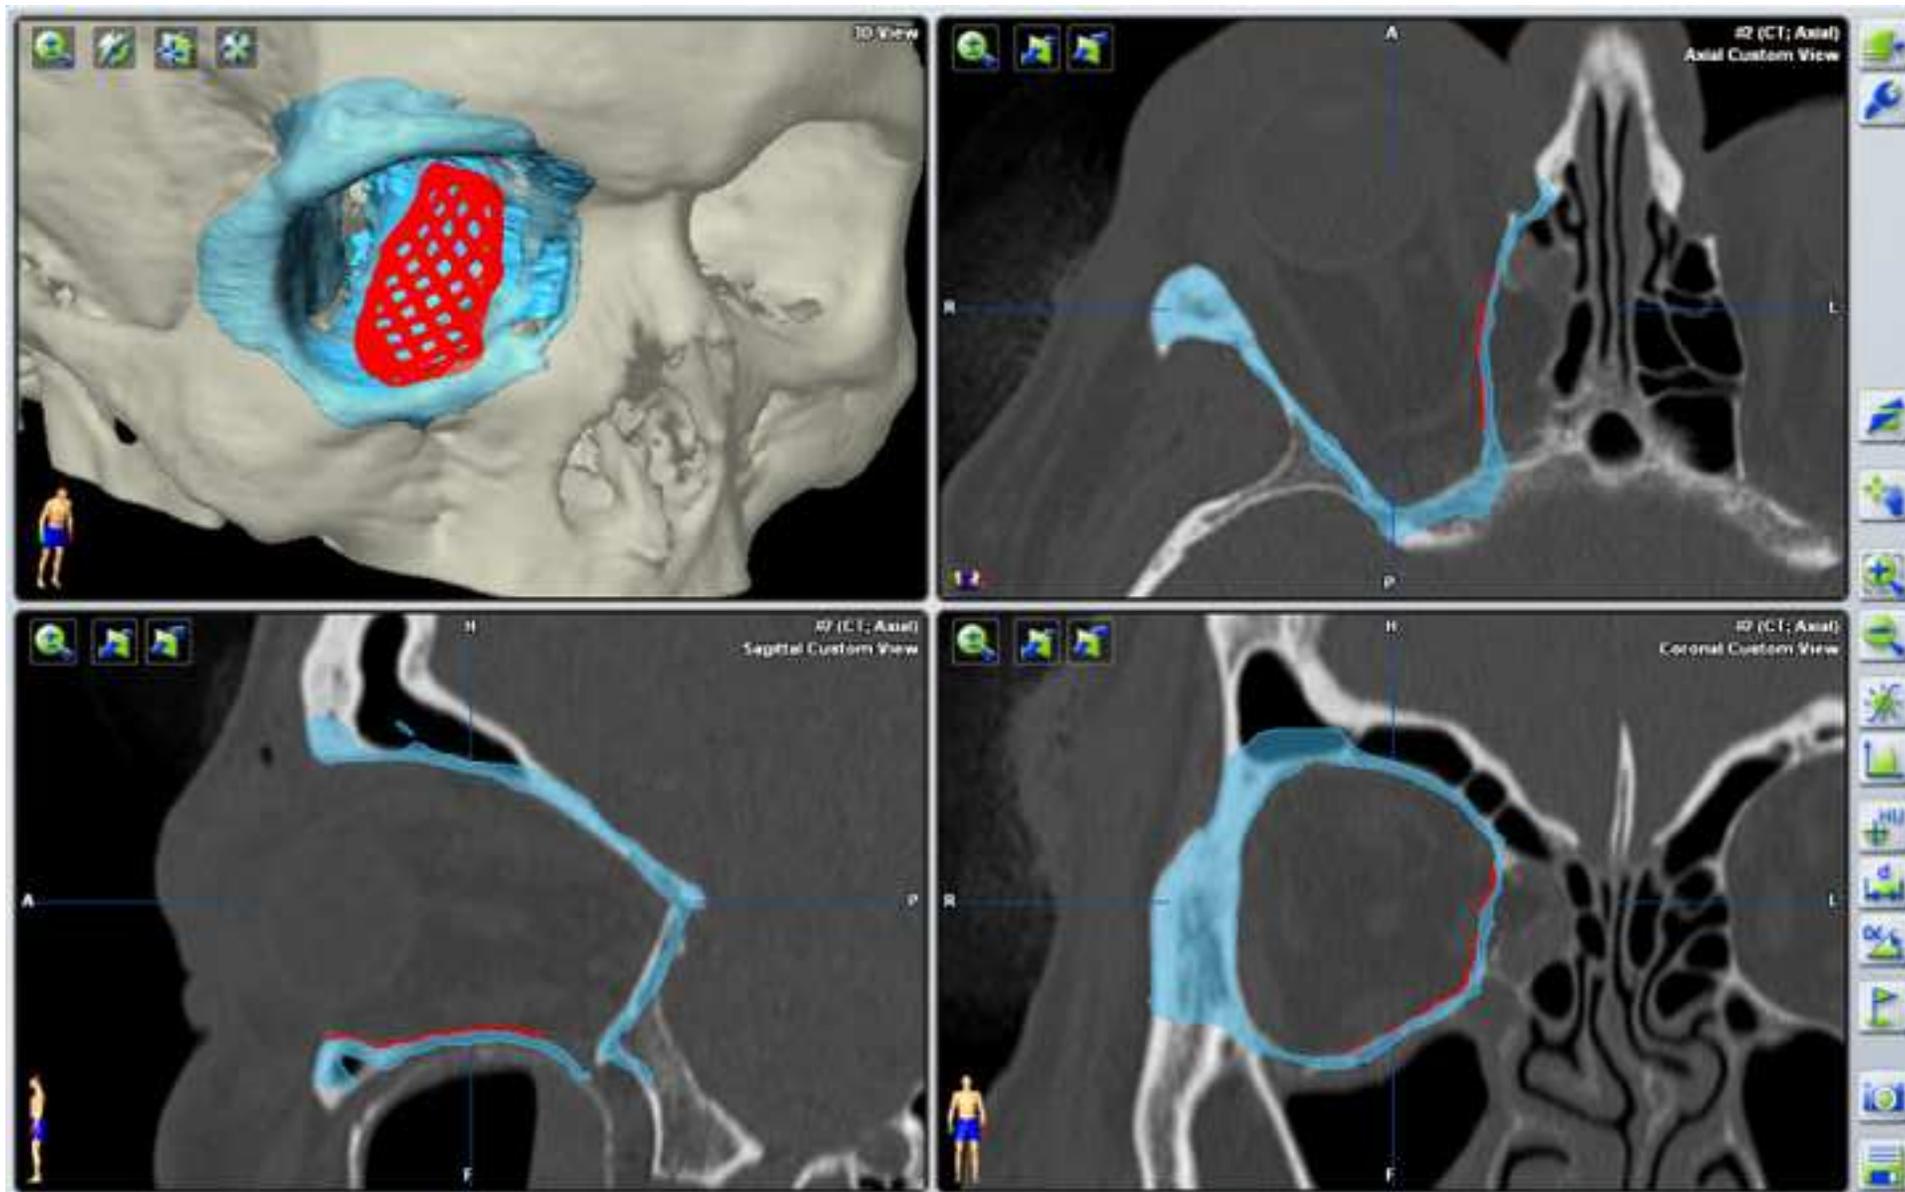


Figure 5
[Click here to download high resolution image](#)

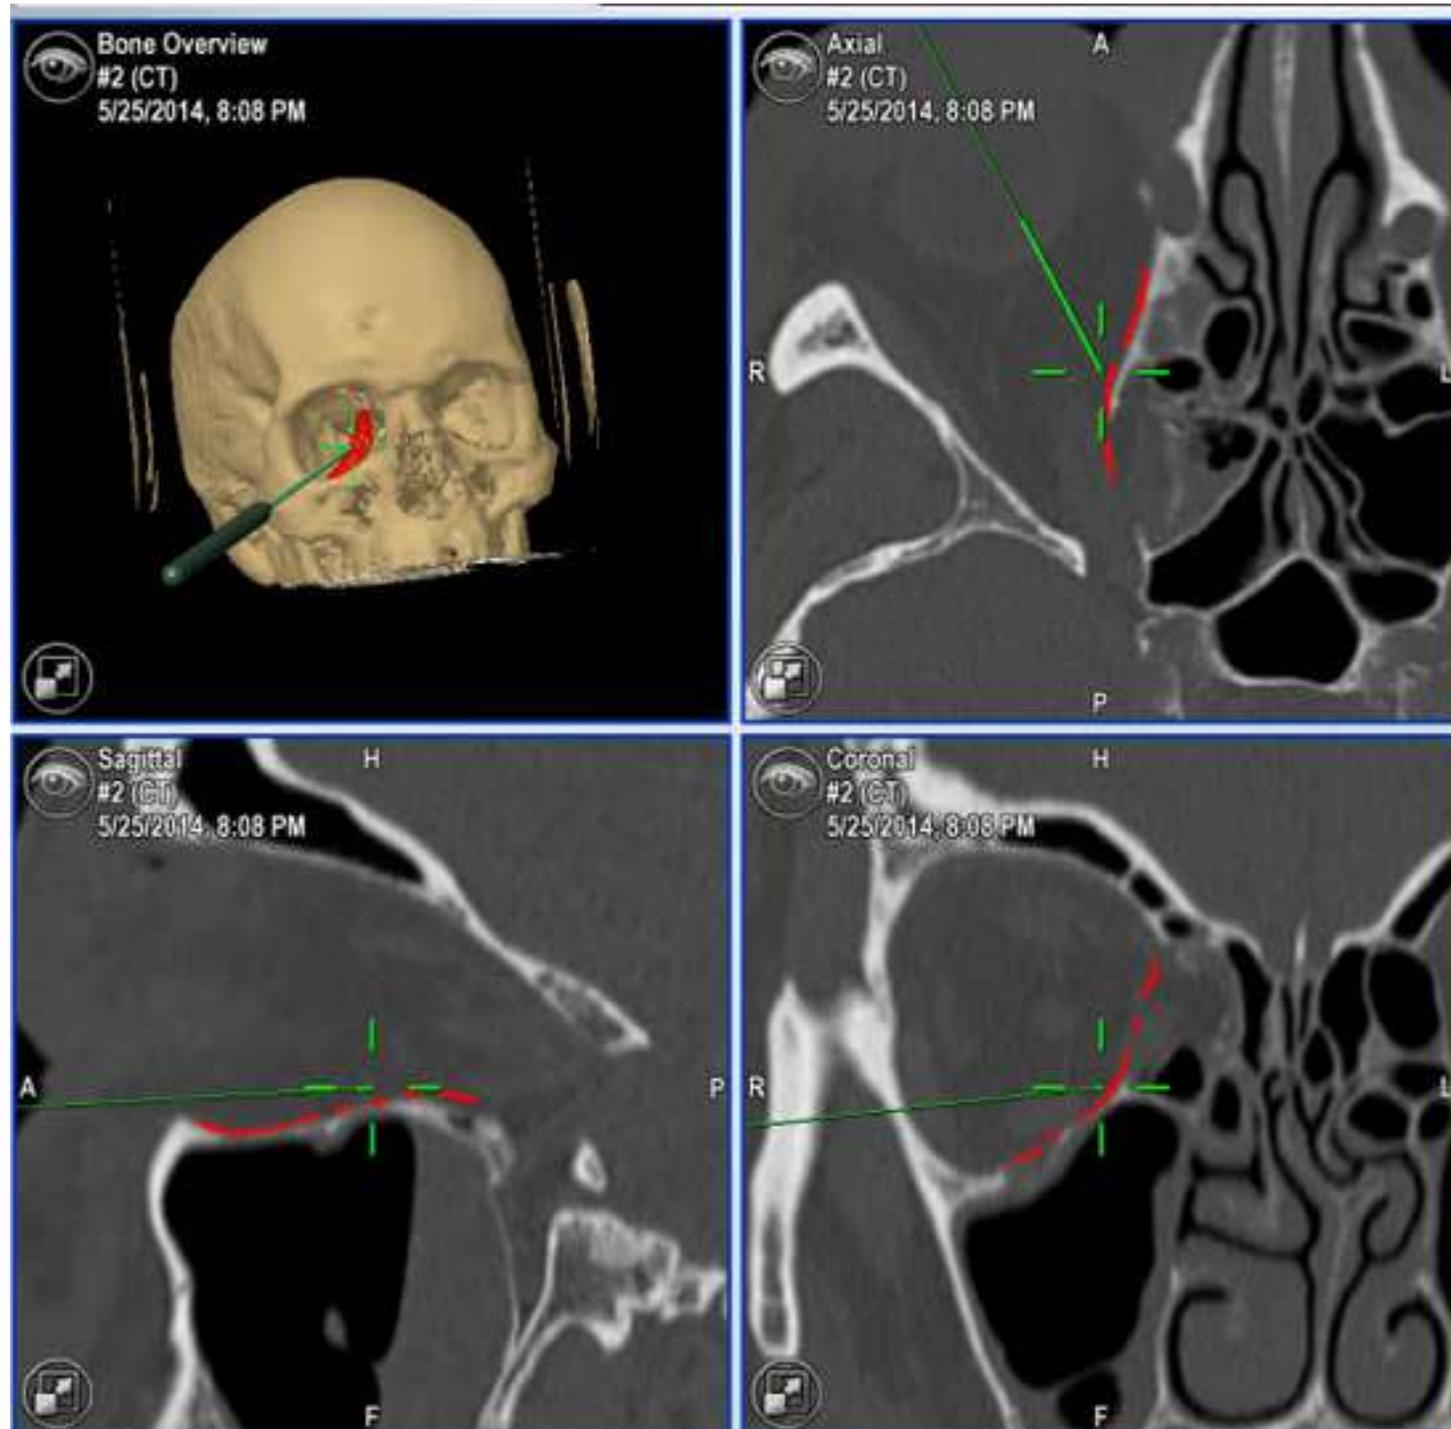


Figure 6
[Click here to download high resolution image](#)


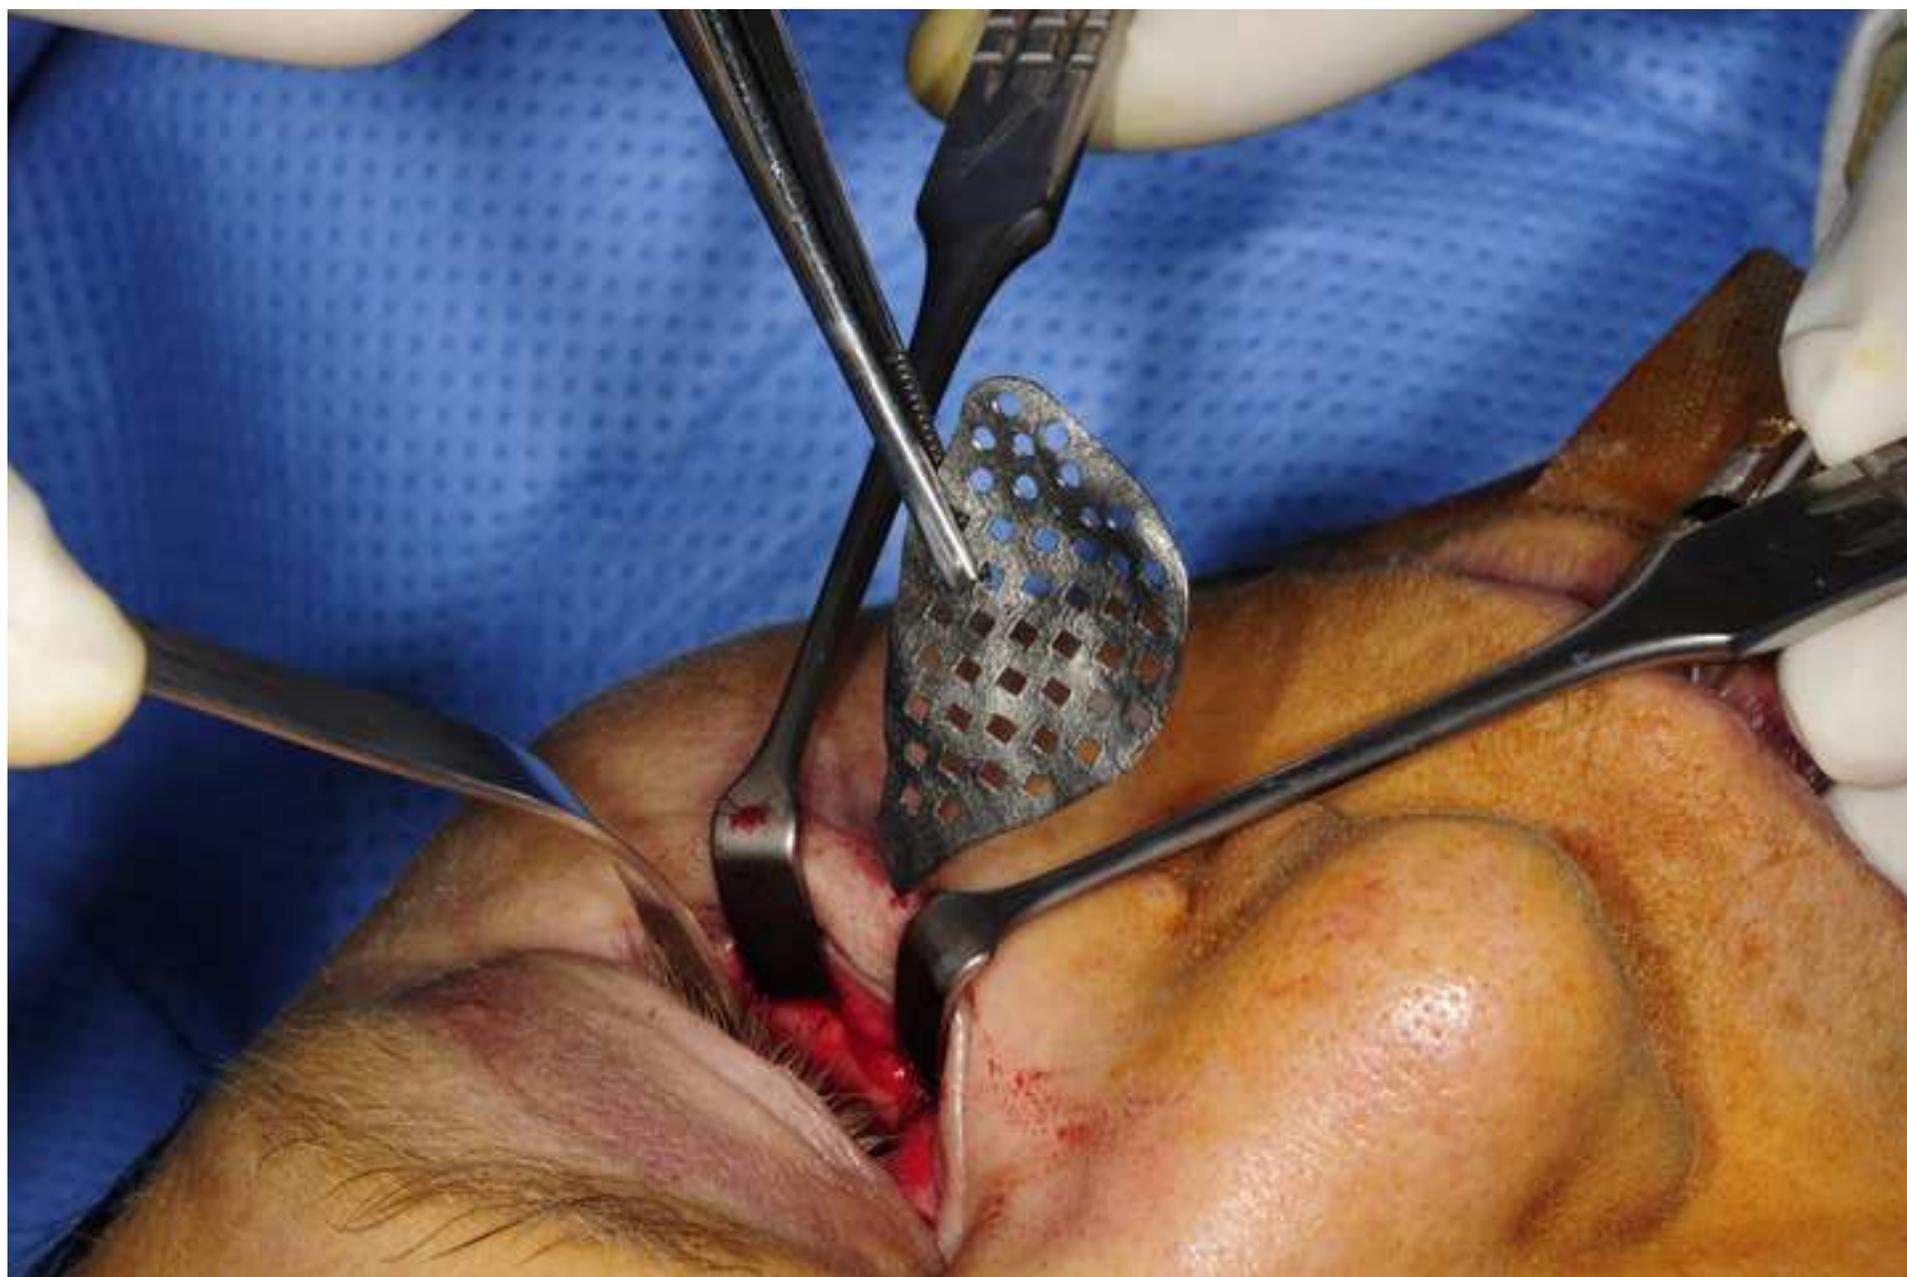


Figure 7
[Click here to download high resolution image](#)

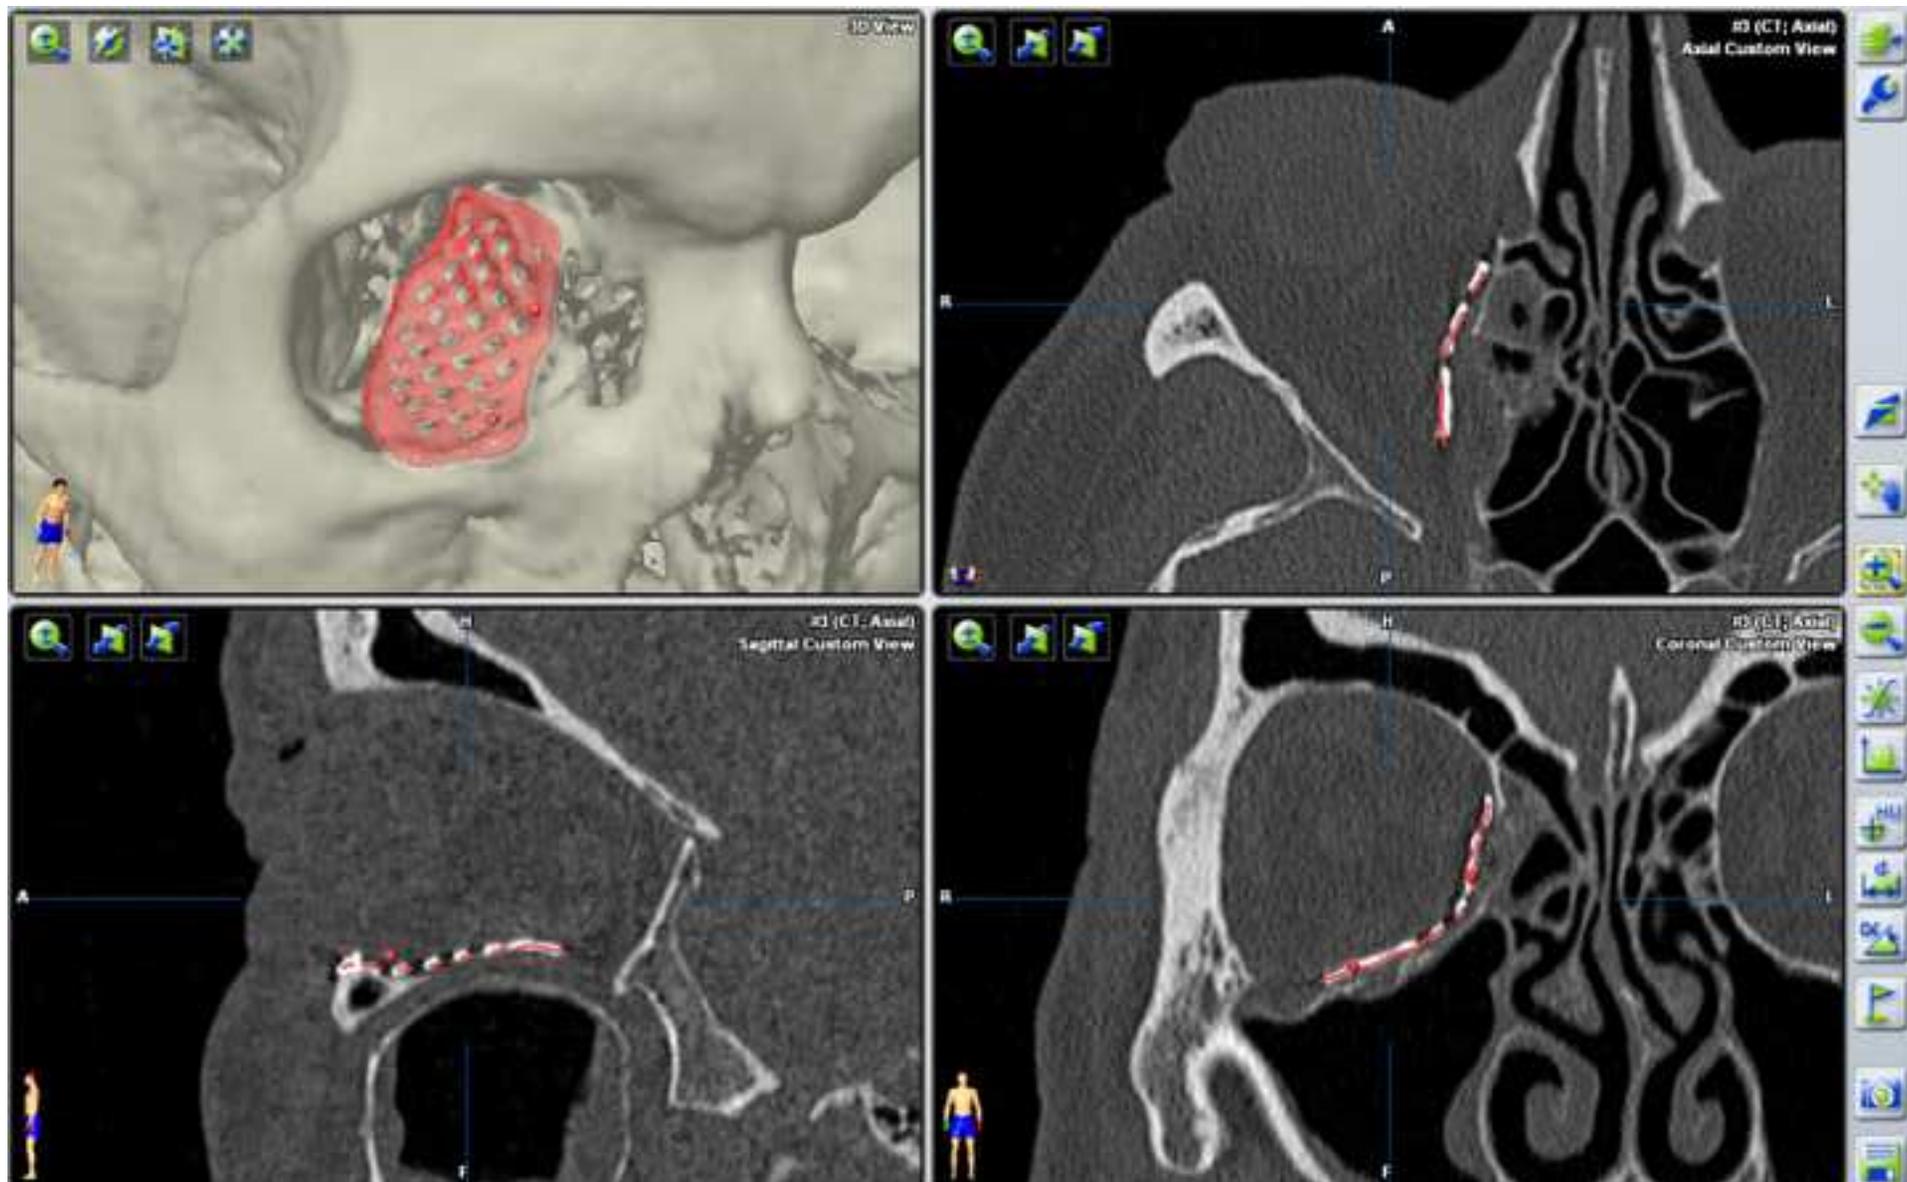

Summary

Fractures of the orbital wall and floor can be challenging due to the demanding three-dimensional anatomy and limited intraoperative overview. Misfitting implants and inaccurate surgical technique may lead to visual disturbance and unaesthetic results. A new approach using individually manufactured titanium implants (KLS Martin, Group, Germany) for daily routine is presented in the current paper. Preoperative CT-scan data were processed in iPlan 3.0.5 (Brainlab, Feldkirchen, Germany) to generate a 3D-reconstruction of the affected orbit using the mirrored non-affected orbit as template and the extent of the patient specific implant (PSI) was outlined and three landmarks were positioned on the planned implant in order to allow easy control of the implant's position by intraoperative navigation. Superimposition allows the comparison of the postoperative result with the preoperative planning. Neither reoperation was indicated due to malposition of the implant and the ocular bulb nor visual impairments could be assessed.

PSI allows precise reconstruction of orbital fractures by using a complete digital workflow and should be considered superior to manually bent titanium mesh implants.

Keywords:

Orbital Fractures; Patient specific Implants (PSI); Reconstruction, Computer-assisted surgery

Patient-Specific Implants in Reconstruction of Orbital Floor and Wall Fractures

Thomas Gander MD, DMD¹

Harald Essig MD, DMD¹

Philipp Metzler MD, DMD¹

Daniel Lindhorst MD, DMD¹

Leander Dubois MD, DMD²

Martin Rücker MD, DMD¹

Paul Schumann MD, DMD¹

¹Department of Oral and Maxillofacial Surgery, University Hospital of Zürich, Zürich, Switzerland

²Department of Oral and Maxillofacial Surgery, University of Amsterdam, Amsterdam, Netherlands

Address of correspondence

Dr. med. Dr. med. dent. Thomas Gander

Department of Oral and Maxillofacial Surgery

University Hospital of Zürich

Frauenklinikstrasse 24

CH-8091 Zürich

Switzerland

Phone 0041442555062

Fax 0041442554179

Email: Thomas.Gander@usz.ch

No sources of support.

Introduction

The orbital wall and floor are common sites of facial bone fracture and may cause serious functional impairment (Shin et al., 2013). Numerous cases of reconstructive implant use have been described in the literature (Strong et al., 2013; Gerressen et al., 2012). The repair of orbital wall and floor fractures is difficult due to the complexity of the anatomical region involved and the limited intraoperative view. Meticulous imaging and clinical examination are indispensable for treatment planning, in order to restore orbital volume and shape. Ill-fitting implants and inaccurate surgical techniques may lead to visual disturbances and unaesthetic results (Ewers et al., 2005). Computer assisted three-dimensional (3D) treatment planning and ready-to-use, individual titanium mesh implants are routinely applied to achieve stable reconstruction and adequate postoperative results (Essig et al., 2013; Schramm et al., 2009). Contemporary standardized titanium meshes are manually adjusted to fit individual patients' polyamide models (Kozakiewicz and Szymor, 2013). We present a new approach using customized, ready-to-use, patient-specific titanium implants (KLS Martin, Group, Germany) suitable for daily use. These easily manufactured and implemented, ready-made patient-specific implants (PSI) allow a more cost-effective and efficient operating procedure.

Material and methods

Patients who underwent operations for orbital wall and/or floor fractures between February 2014 and June 2014 were recruited, irrespective of their gender, age, trauma type, or the presence of concomitant injuries. Informed consent was provided by all patients. Preoperative computed tomographic (CT) scan data, with a slice thickness of 0.3 mm, were processed using the iPlan software package (ver. 3.0.5, Brainlab, Feldkirchen, Germany) to generate a 3-dimensional (3D) reconstruction of the affected orbit, using the mirrored, non-affected orbit as a template. Correction of minor asymmetry was effected via the 3D smart shaper function. Accurate use of the 3D smart shaper is a key step in the planning process, and must be performed with caution to avoid discrepancies during subsequent implant placement (Figures 1-2). The parameters of the PSI are outlined, and three landmarks are positioned on the planned implants to allow rapid and effective 3D control of the implant's position (Figures 3-5). Each planning step can be easily performed by any surgeon: no specialist is needed, although *a priori* knowledge of the software is beneficial.

Precise transfer of the 3D coordinates of the implant, from iPlan 3.0.5 to the manufacturing software (KLS Martin), represents an essential precondition of intraoperative control. STL data are then exported and approved for the purposes of implant manufacture. This procedure obviates the need for time-consuming integration of the dataset within the manufacturing software. Circumferential implant cushions should be created, although laser-sintered, individually manufactured implants (with a thickness of 0.3 mm) exhibit greater stiffness compared with manually adjusted titanium meshes and therefore allow minor dimensioning of the implant (Ibrahim et al., 2009). Overextended PSI can easily be reduced in extent by pincers and manual adjustment is still possible, although to a lesser degree

compared with standardized implants. The need of manual adjustment should be avoided by meticulous preoperative implant planning.

Individually manufactured titanium implants are positioned using a retroseptal, transconjunctival approach (Figure 6). Application of a polydioxanon foil, which may improve the surgeon's view by preventing fatty tissue from encroaching on to the operative site, can be utilized in certain cases. The polydioxanon foil is removed following placement of the implant and prior to wound closure. Dental arch splints in dentulous patients, and mini screws placed in the calvarian bones of edentulous patients, were used as registration markers. Postoperative CT scans were performed to assess implant position. Quality management was effected by importation and superimposition of the postoperative dataset (Figure 7). All patients underwent a pre- and post-operative ophthalmological examination.

Results

A total 12 patients were included. All patients underwent reconstruction of the orbital wall or orbital floor, via PSIs using intraoperative navigation, and in accordance with a transconjunctival, post-septal approach. In eight patients, the indication for surgery was imposed due to diplopia. Four patients underwent orbital reconstruction owing to profound defects or enophthalmos. The male to female ratio of the sample was 11:1, with a mean age of 53 years (range: 29-78 years). Major causes of orbital floor or wall fractures included industrial accidents and falls (Table 1).

In seven patients, dental splints were applied for intraoperative navigation purposes, in addition to dental cusps. In four patients, navigation screws were employed in the calvaria, for intraoperative registration and navigation. CT scans were performed preoperatively, and the registration tools were introduced.

The time taken for digital planning ranged between 30 and 36 min: the manufacturing process took 4-6 days. All individually manufactured implants were placed without difficulty. Postoperative CT scans revealed accurate fitting of the PSI. No visual impairments were reported aside from double vision in terminal positions, which resolved during postoperative care. Reoperation was not required to reposition implants or to correct displacement of the ocular bulb. In two cases, intraoperative reduction of the implant, using pincers, was necessary due to overextension during computer-aided treatment planning. **Manual adjustment by bending was not necessary in any case.** Patients did not report sensations indicative of foreign bodies or any visual impairment (Table 2).

Discussion

Orbital floor and wall fractures represent common skeletal, facial injuries (Rosado and de Vicente, 2012; Dimitroulis and Eyre, 1991): diplopia, enophthalmos and infra-orbital and optical nerve injuries are potential complications of orbital floor and wall fracture surgery (Brucoli et al., 2011). Safe, rapid, reproducible, and precise procedures are required to avoid such issues. Computer-assisted surgery represents a key step towards safer practice and has become a standard technique during the past few years, allowing virtual surgery planning, simulation, and intraoperative control (Essig et al., 2013; Schramm et al, 2009). New surgical methods and improved implant designs and materials have been introduced incrementally, in some cases with great success (Gierloff et al., 2012; Avashia et al., 2012; Ciprandi et al., 2012; Schumann et al., 2013). PSIs allow the precise reconstruction of orbital fractures by means of a complete digital workflow. Manually bent titanium mesh implants will become less important. A precondition of the digital workflow is the

transfer of the planning software's coordinates system into the manufacturing software, to avoid time-consuming and erroneous positioning of the virtual implant. Correct positioning of the PSI can be verified using intraoperative navigation, to support the three virtually planned indentations incorporated in the manufactured implant (Schramm et al., 2009). The three planned indentations and their stored coordinates also serve as measuring points during the virtual planning process, thereby improving overall accuracy. The implant is digitally planned by the surgeon, with a focus on its extent and the position of the three landmarks. The coordinate system of the digital plan must be conserved during the entirety of the manufacturing process, to allow accurate superimposition of the pre- and postoperative implant positions. Although PSIs are dimensionally more stable compared with manually bent titanium implants, a circumferential cushion is nonetheless recommended. Furthermore, stiffness in PSIs prevents implant deformation during placement, but still allows minor intraoperative corrections by pincers. Due to the increased stiffness of laser-sintered PSIs compared with conventional titanium meshes, precise preoperative planning is required to avoid interference during insertion of the PSI. Routinely incorporating postoperative results into preoperative virtual planning activities, and assessing implant positioning via superimposition, both represent ground-breaking advances in medical quality control.

Conclusion

PSIs simplify the reconstruction of orbital floor and wall fractures, and should be considered a more accurate alternative to manually bent titanium mesh implants. Automation allows the application of safe, time-effective, daily procedures; accordingly, its use should be encouraged. Implant planning can be easily

undertaken by any surgeon, and does not require specialized, software-specific knowledge.

As previously stated by the World Health Organization, PSIs should play a key role in daily routines, and furthermore should replace conventional implants by 2020. PSI for the reconstruction of orbital floor and wall fractures are now readily available.

More patients will be included in this study, and long-term results will be gathered in the future to allow more funded statements.

Conflict of Interest Statement

All authors disclose any financial and personal relationships with other people or organisations that could inappropriately influence (bias) this work.

Funding

None.

References

Shin JW, Lim JS, Yoo G, Byeon JH: An analysis of pure blowout fractures and associated ocular symptoms. *J Craniofac Surg* 24:703-707, 2013.

Strong EB, Fuller SC, Wiley DF, Zumbansen J, Wilson MD, Metzger MC: Preformed vs intraoperative bending of titanium mesh for orbital reconstruction. *Otolaryngol Head Neck Surg* 149:60-66, 2013.

Gerressen M, Gillessen S, Riediger D, Hölzle F, Modabber A, Ghassemi A: Radiologic and facial morphologic long-term results in treatment of orbital floor fracture with flexible absorbable alloplastic material. *J Oral Maxillofac Surg* 70:2375-2385, 2012.

Ewers R, Schicho K, Undt G, Wanschitz F, Truppe M, Seemann R, Wagner A: Basic research and 12 years of clinical experience in computer-assisted navigation technology: a review. *Int J Oral Maxillofac Surg* 34:1-8, 2005.

Essig H, Dressel L, Rana M, Kokemueller H, Ruecker M, Gellrich NC: Precision of posttraumatic primary orbital reconstruction using individually bent titanium mesh with and without navigation: a retrospective study. *Head Face Med* 9: 18, 2013.

Schramm A, Suarez-Cunqueiro MM, Rücker M, Kokemueller H, Bormann KH, Metzger MC, Gellrich NC: Computer-assisted therapy in orbital and mid-facial reconstructions. *Int J Med Robot* 5:111-124, 2009.

Kozakiewicz M, Szymor P: Comparison of pre-bent titanium mesh versus polyethylene implants in patient specific orbital reconstructions. *Head Face Med* 29:32, 2013.

Ibrahim D, Broilo TL, Heitz C, de Oliveira MG, de Oliveira HW, Nobre SM, Dos Santos Filho JH, Silva DN: Dimensional error of selective laser sintering, three-dimensional printing and PolyJet models in the reproduction of mandibular anatomy. *J Craniomaxillofac Surg* 37:167-173, 2009.

Rosado P, de Vicente JC: Retrospective analysis of 314 orbital fractures. *Oral Surg Oral Med Oral Pathol Oral Radiol* 113:168-171, 2012.

Dimitroulis G, Eyre J: A 7-year review of maxillofacial trauma in a central London hospital. *Br Dent J* 20:300-302, 1991.

Brucoli M, Arcuri F, Cavenaghi R, Benech A: Analysis of complications after surgical repair of orbital fractures. *J Craniofac Surg* 22:1387-1390, 2011.

Gierloff M, Seeck NG, Springer I, Becker S, Kandzia C, Wiltfang J: Orbital floor reconstruction with resorbable polydioxanone implants. *J Craniofac Surg* 23:161-164, 2012.

Avashia YJ, Sastry A, Fan KL, Mir HS, Thaller SR: Materials used for reconstruction after orbital floor fracture. *J Craniofac Surg* 23: 1991-1997, 2012.

Ciprandi MT, Primo BT, Gassen HT, Closs LQ, Hernandez PA, Silva AN Jr: Calcium phosphate cement in orbital reconstructions. *J Craniofac Surg* 23: 145-148, 2012.

Schumann P, Lindhorst D, Wagner ME, Schramm A, Gellrich NC, Rucker M: Perspectives on resorbable osteosynthesis materials in craniomaxillofacial surgery. *Pathobiology* 80: 211-217, 2013.

Tables/Figures

Table 1 Patient data

Table 2 Results

- Figure 1 Placement of the smart shaper in the required area.
- Figure 2 Adaptation of the selected area with the smart shaper.
- Figure 3 Determination of the prospective implant's extent.
- Figure 4 Implant design.
- Figure 5 Intraoperative navigation for implant position control.
- Figure 6 Transconjunctival, post-septal patient-specific implant (PSI) placement.
- Figure 7 Superimposition of the preoperative planning position upon the postoperative patient-specific implant (PSI) position.

The English in this document has been checked by at least three professional editors, all native speakers of English.